

NAAC  
REACCREDITED

# C. U. Shah College of Pharmacy S. N. D. T. Women's University, Mumbai.

Sir Vithaldas Vidya Vihar, Santacruz (West), Mumbai - 400 049.

E-mail : cushahpharmacy@sndt.ac.in Telegram : SHAHPHARMA

Tel. : 2660 8493, Extn. : 2239 (D) : 2660 9577



**DR. (MRS.) PRATIMA A. TATKE**  
Principal

## Web notification for Invitation of Quotation of Purchase of Dissolution Testing Apparatus

Ref. No.: CUP-276/21-22/ 195

Date: 24/12/21

Sealed Quotations are invited for purchase of **Dissolution Testing Apparatus** at **C. U. Shah College of Pharmacy, Juhu Campus, Santacruz (W), Mumbai-400049**. The Suppliers should strictly adhere to the terms and conditions as per the Specifications. The University reserves the right to reject the quotations in whole without assigning any reason thereof.

Name of Item	Dissolution Testing Apparatus
Venue of submission	C. U. Shah College of Pharmacy, SNDT Women's University, Juhu campus, Santacruz (W), Mumbai-400049
To be addressed to	Principal
Contact Telephone	22 26608493/ 22 26608462 Extn: 2239
Dead line of submission	31 <sup>st</sup> December, 2021

### Instructions:

Dates mentioned here are scheduled dates for the University activities. Any changes in date of submission and processing shall be filed in Tender/Quotations Section on the University website (sndt.ac.in). Quotations should also mention all technical specifications as mentioned in this document.

The quotations are invited for the product: Dissolution Testing Apparatus

### Specifications:

- Baskets with rod (USP I) 08, Paddles (USP II) 08 nos, Clear merlon jars with lids 08
- Isolated water circulating pump 01, Moulded water bath 01, External temperature probe
- Speed range: Variable speed from 20 to 300 RPM, Speed accuracy:  $\pm 0.5$  RPM
- Temperature range: 20° C to 40°C, Temperature accuracy:  $\pm 0.1$  °C, Display: 40 x 4 character backlighted LCD
- No. of protocol: 20 maximum, Sample interval: Maximum 24 of 1 min to 23 hrs, 59 min
- Bath: Clear acrylic moulded water bath, Bath size (L x W x H): (705 x 374 x 200) mm, Heater: 1 kW/230 VAC, material S.S. 304 with sensor
- Pump supply: 230 VAC, 50 Hz, Pump type: Magnetic coupling Pump flow rate: 10 litres/minute maximum, Power supply: 220/ 230 VAC, 50/60 Hz, 1.3 kW/6 Amp Dimensions (L x W x H): (705 x 505 x 645) mm

The quotations are invited in two parts under three envelop system. The Technical specifications envelop shall be enclosed and sealed in envelop No-1. Schedule of rates shall be filled in and enclosed in envelop No-2. Both sealed envelopes shall be kept in envelop No-3. On each envelop name and address along with contact number of bidder shall be written.

### Envelop No.1 must contain:

- a) Covering letter with details of bidder, name of proprietor, Telephone number, Mobile number, email ID signature with seal.
- b) Type of business entity: manufacturer / authorized dealer, any other
- c) Certified copy of GST registration
- d) Pan Card No:

### Envelop No. 2 must contain:

The financial bid may be submitted in the prescribed format as below on the letter head of the bidder.


3. Format as below on the letter head of the bidder.

Item (With all specifications, Make and Model no)	Rate per unit (INR)	Taxes (INR)	Qty (Total 1)	Total estimated cost (INR)
---	---------------------	-------------	---------------	----------------------------

The rate must be inclusive of all charges. Taxes are to be mentioned clearly in the quotation free delivery; free installation will be done at C.U.Shah College of Pharmacy, SNDT Women's University Juhu Campus.

The rate validity will be upto 90 days from the date of submission deadline.

All necessary documents, manuals to be handed over to C.U.Shah College of Pharmacy, SNDT Women's University, Juhu Campus, Santacruz (W), Mumbai 400049

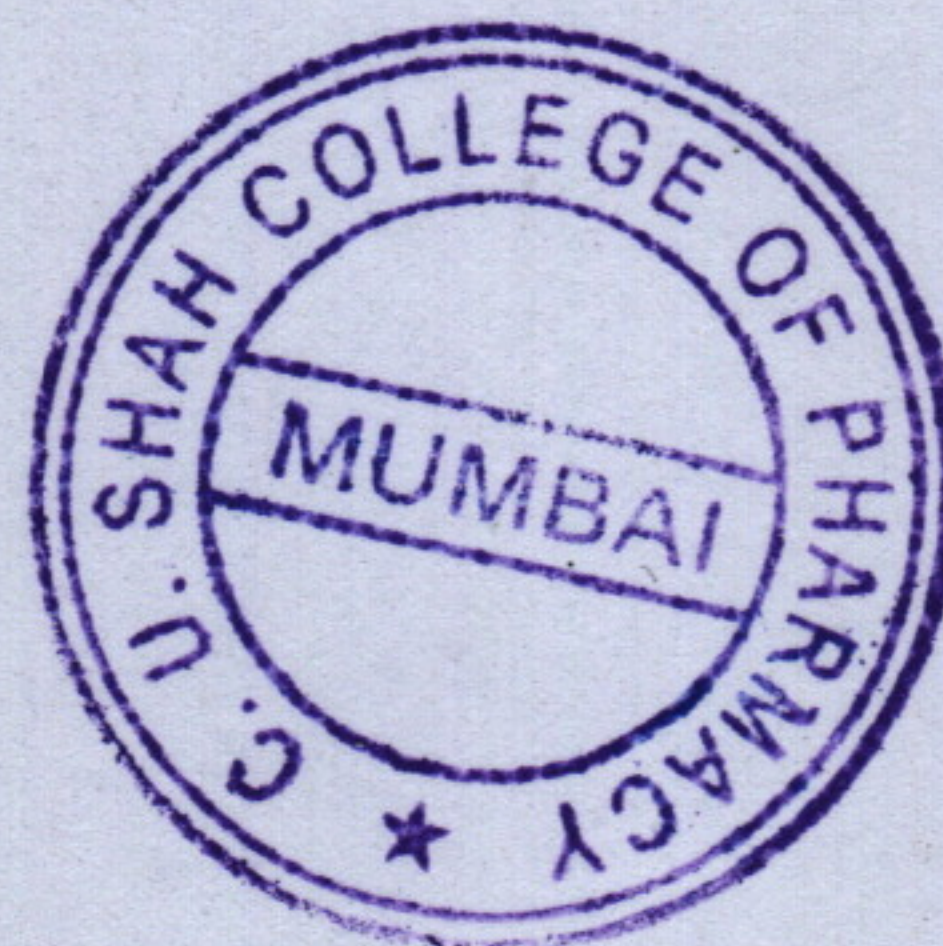

*Pratika*  
Dr. Pratima Tatke  
Principal and Professor

*Pratika*  
Dr. Pratima Tatke  
Principal

C. U. Shah College of Pharmacy,  
S.N.D.T. Women's University,  
Santacruz (W), Mumbai - 400 049.

The College has the facility of C. U. Shah Pharmaceutical Research Centre